

10072020-020502





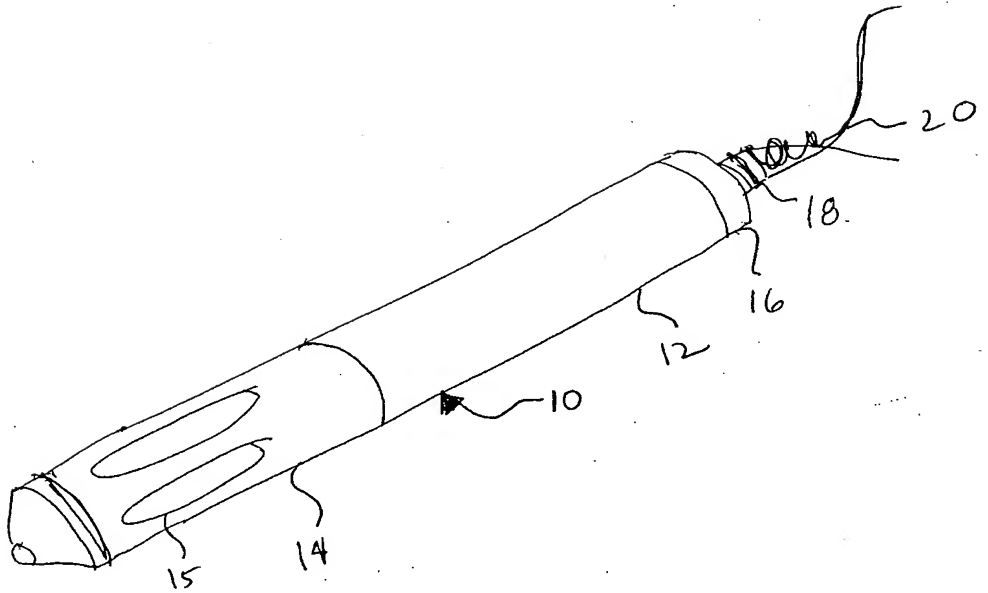


FIG. 1a

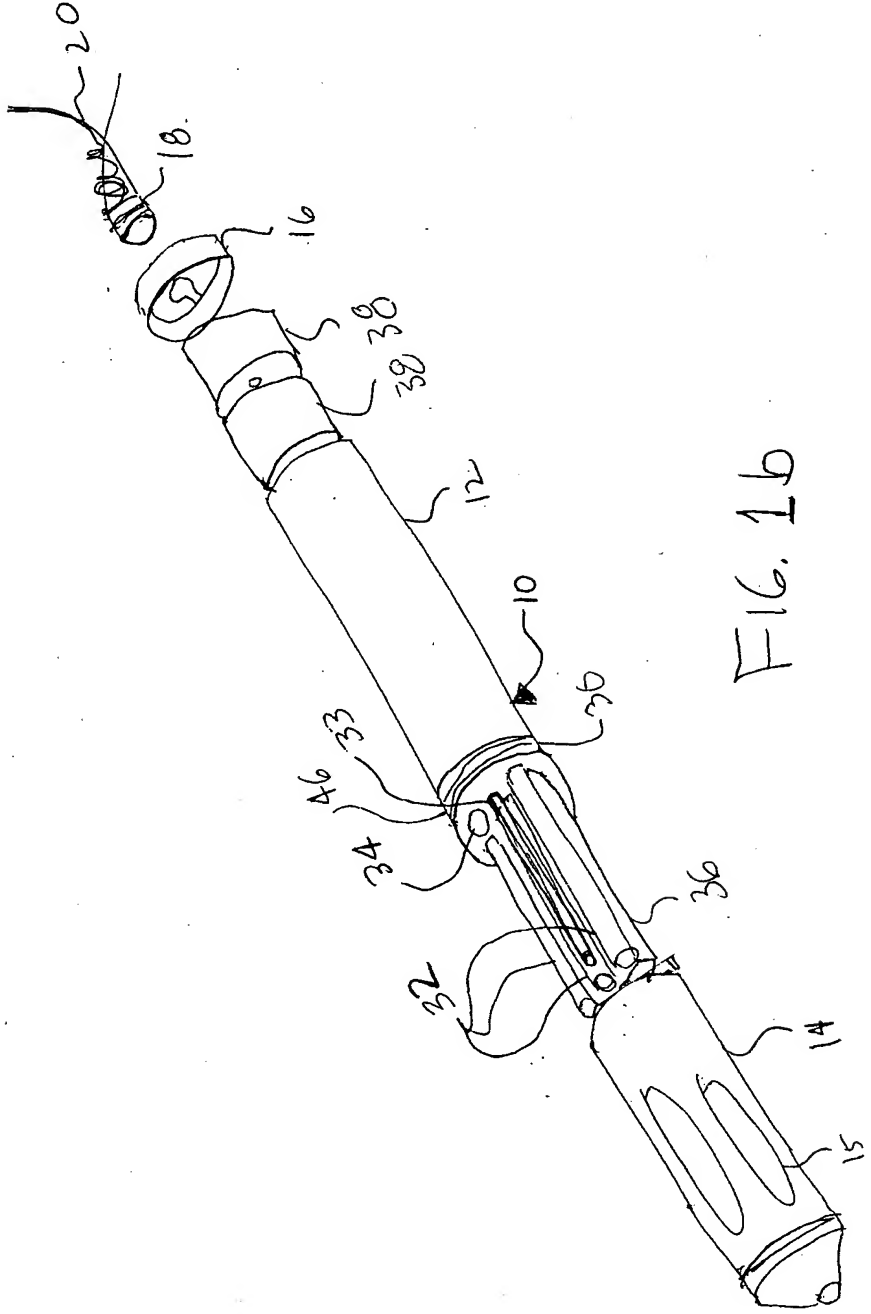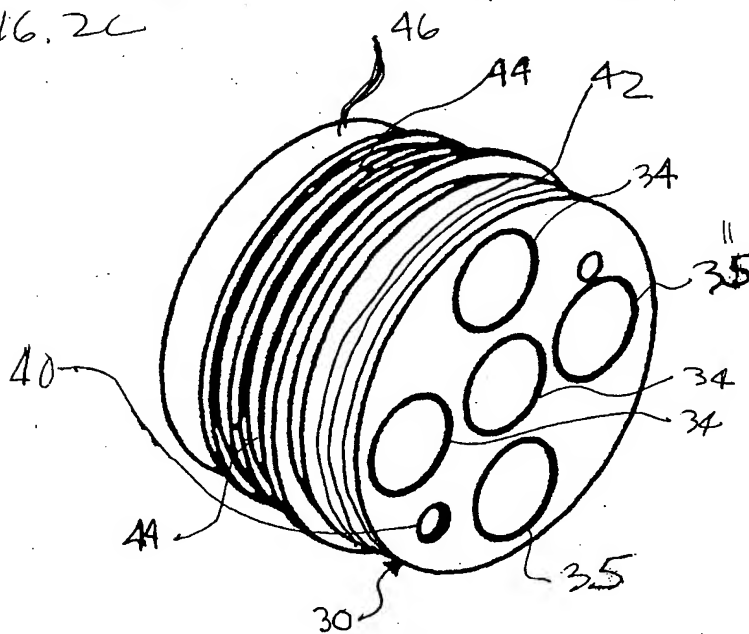
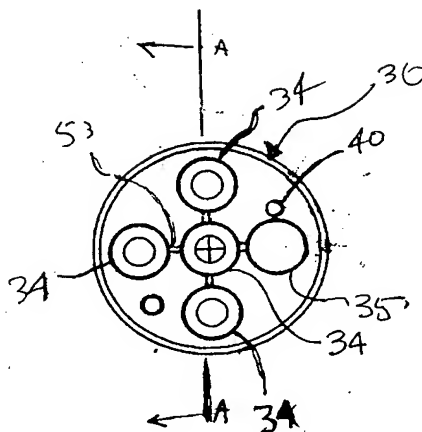


10072020-0206501

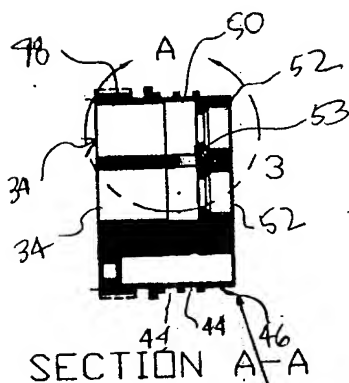

10072020-020502

10072020-020502

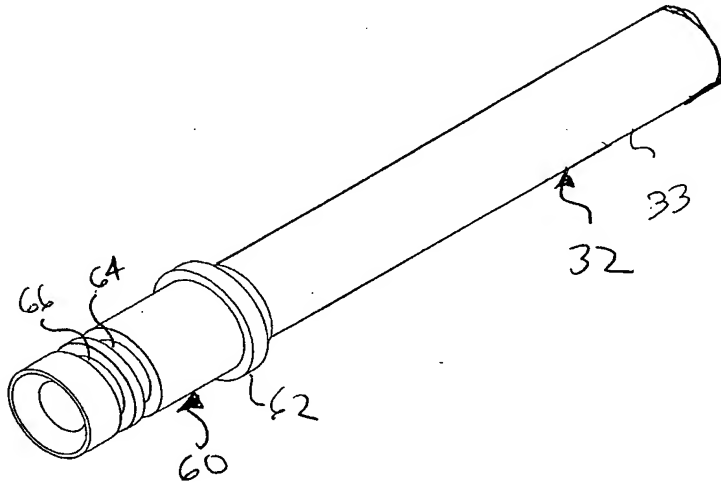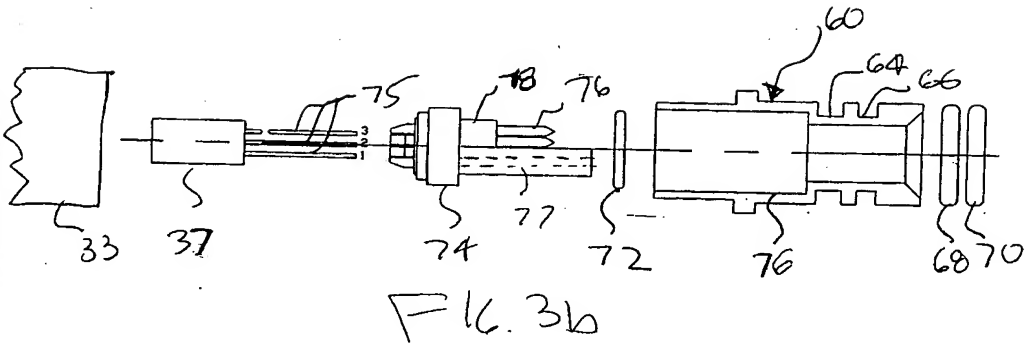

10072020-020601




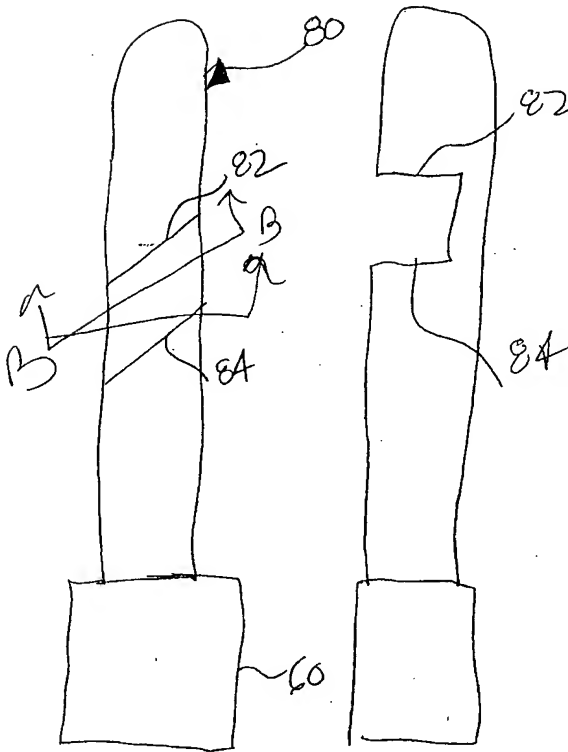



FIG. 4a

FIG. 4b

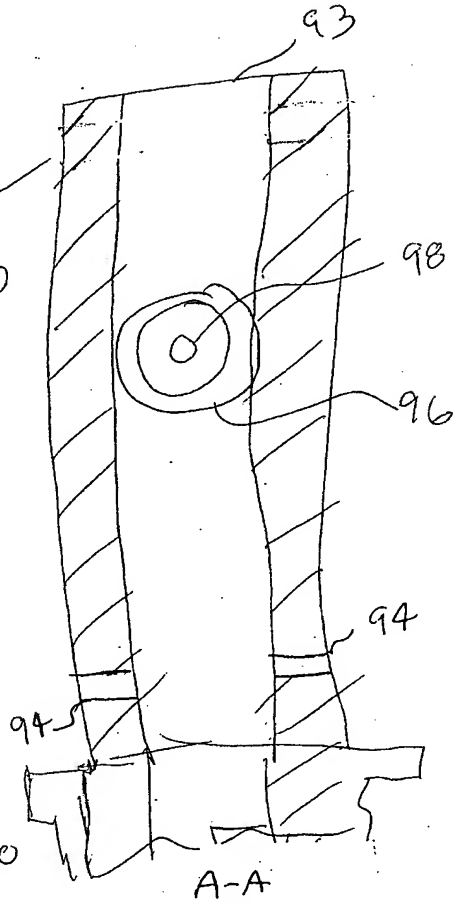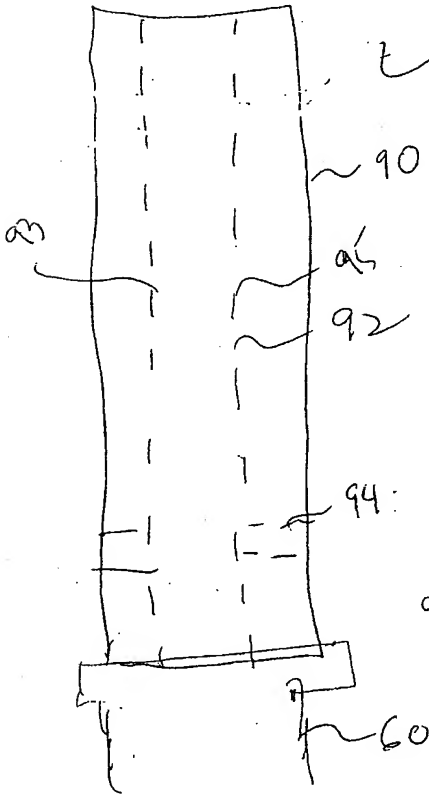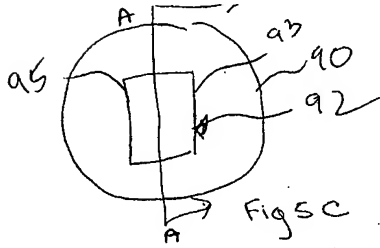

10072020-020602

10072020-020662

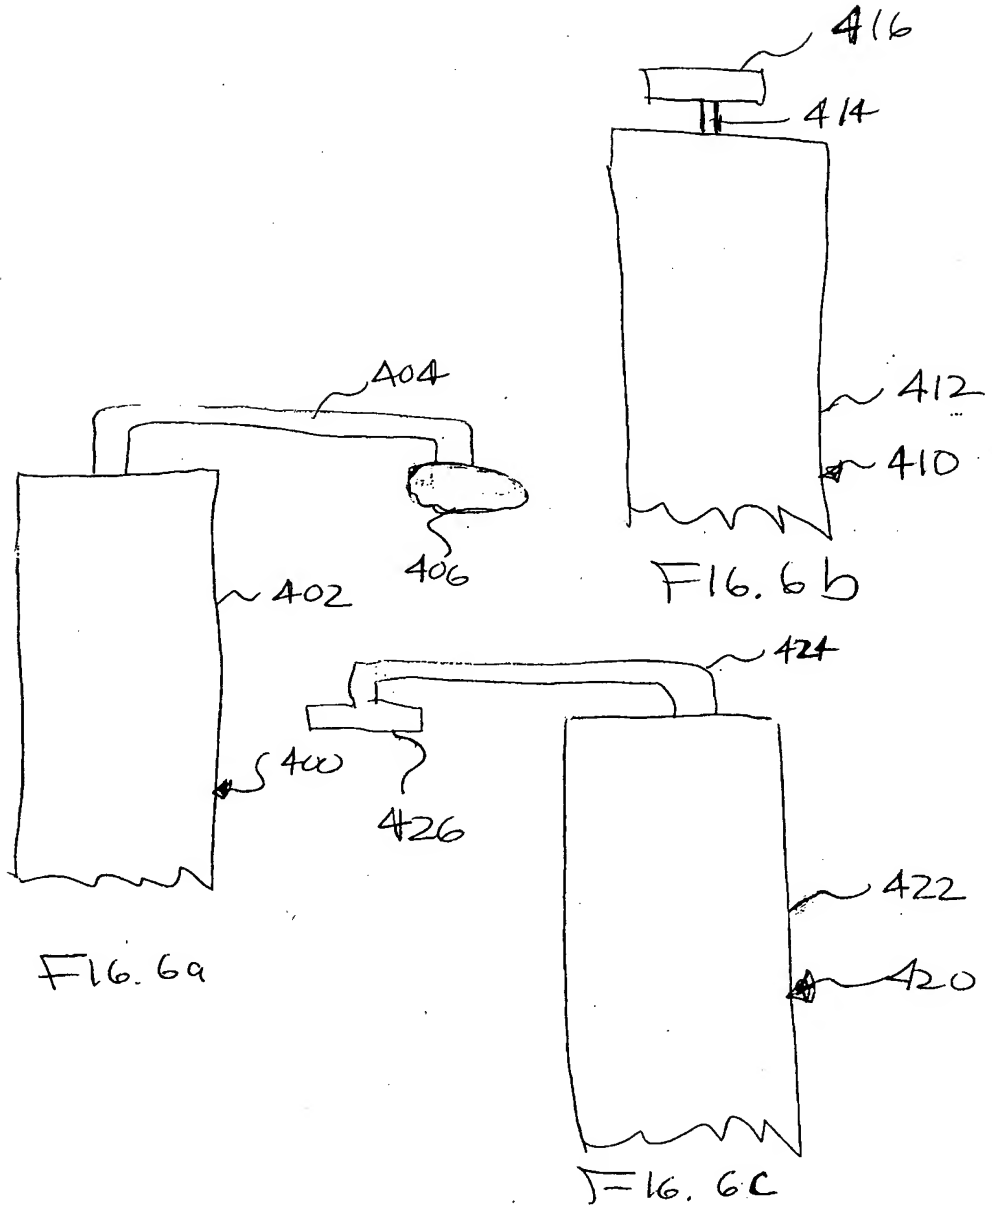

10072030-020602


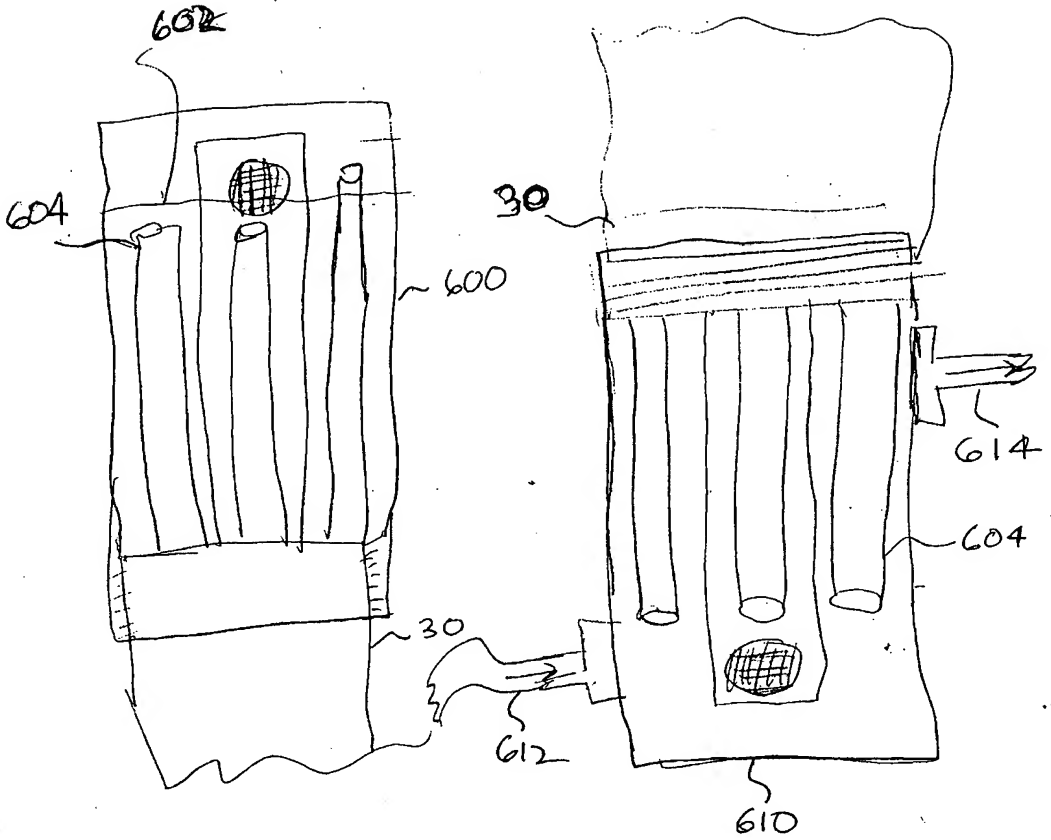


FIG. 7a

FIG. 7b




10072020-020602

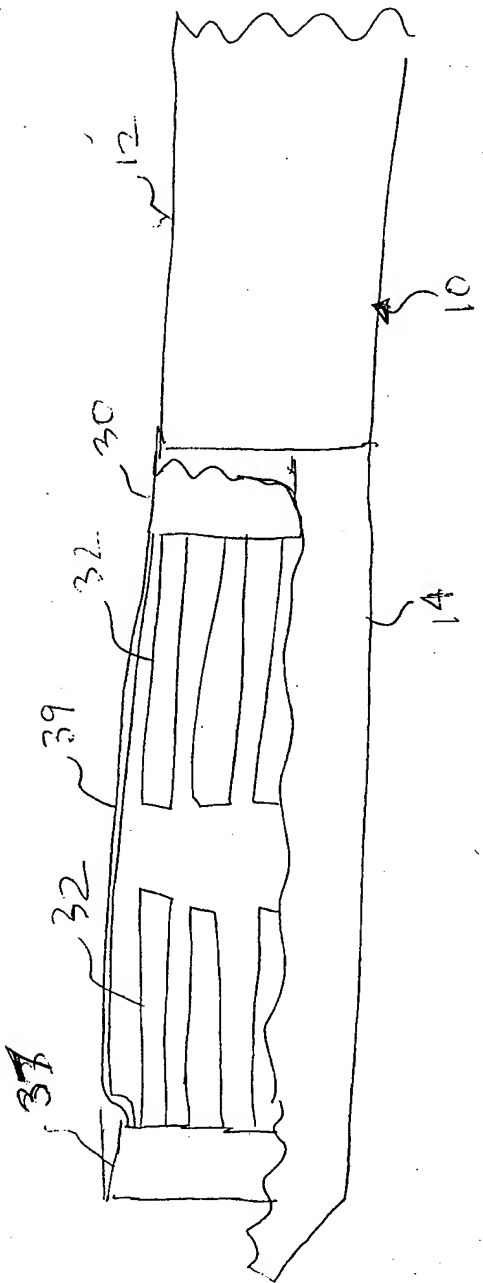

F16.8a

10072020-020502

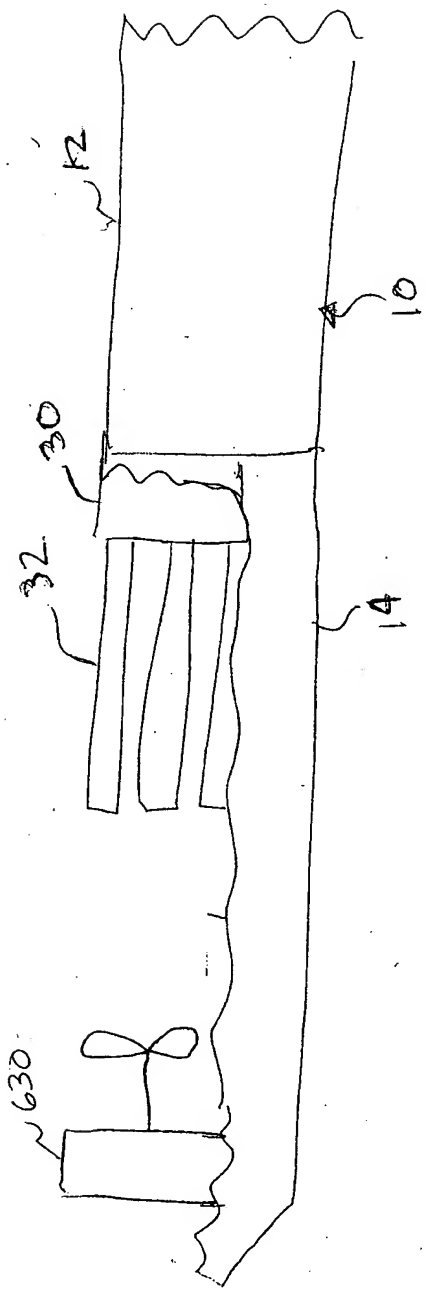

F16.8b


Title: "SENSOR HEAD APPARATUS"

Applicant: [REDACTED] D. Henry, Ph.D., et al.

Docket No. 74-00392

Express Mail No.: EL702178314US

Attorney: Kenneth J. Johnson, Tel: (303) 338-0997

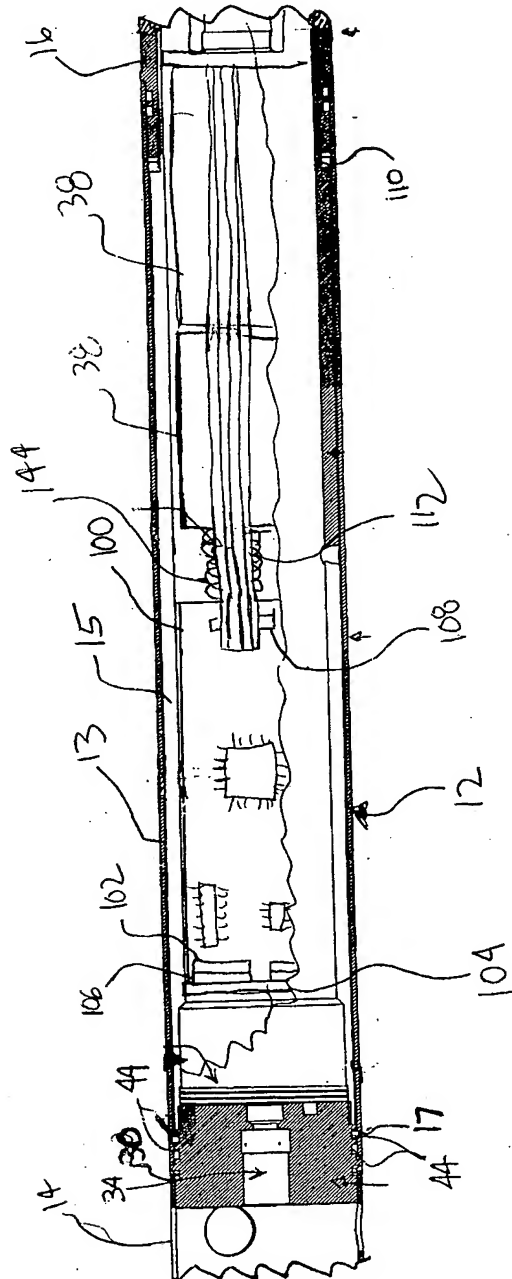

419

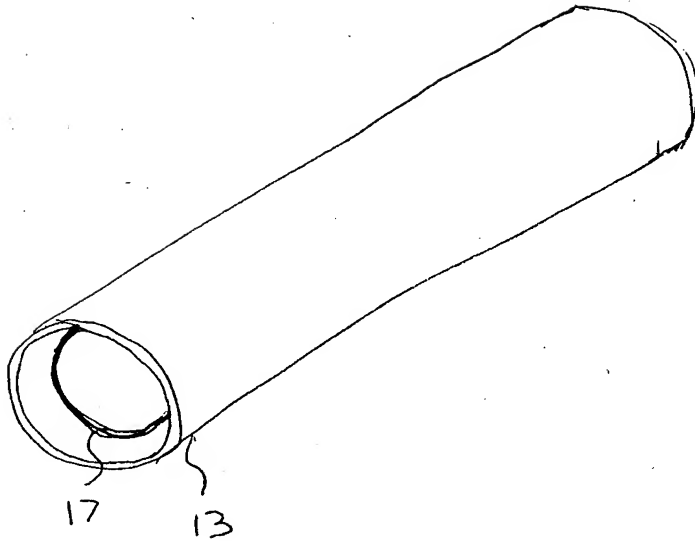


FIG. 10

10072020-020502




FIG. 11b

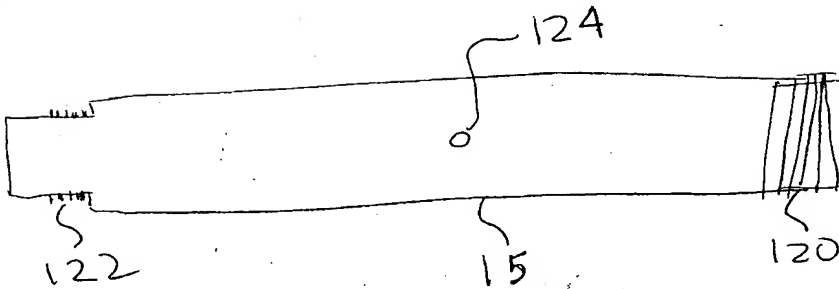


FIG. 11a

10072020-020502

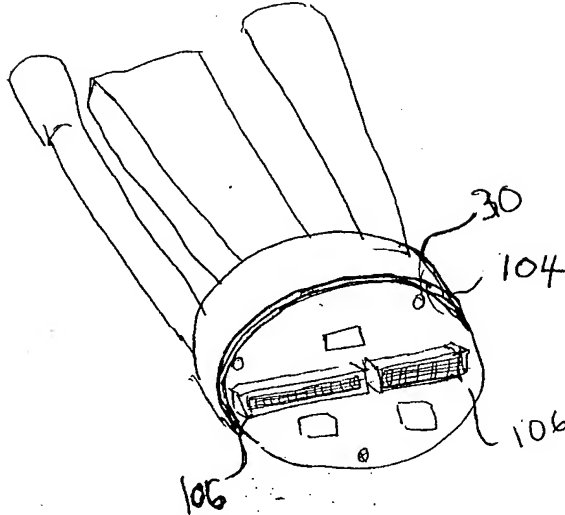


FIG. 12a

10072020-020502


Title: "SENSOR HEAD APPARATUS"

Applicant: Dr. D. Henry, Ph.D., et al.

Docket No.: 74-00392

Express Mail No.: EL702178314US

Attorney: Kenneth J. Johnson, Tel: (303) 338-0997

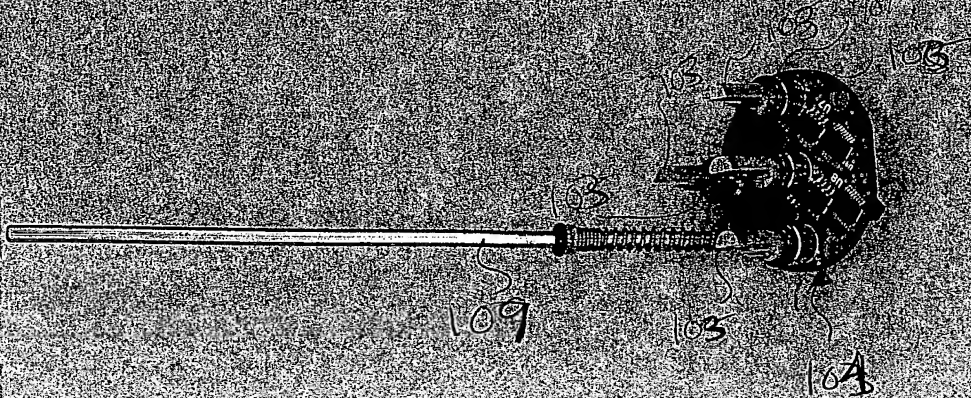

F16.12b


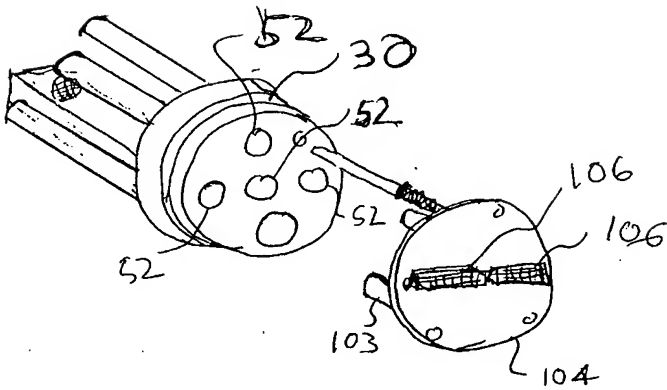





FIG. 12C

10072020.020600





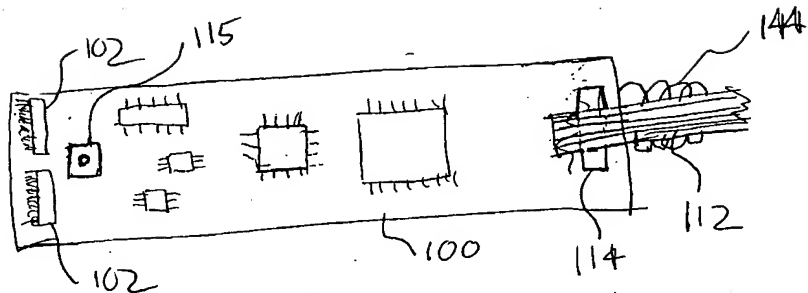

10072020-020502

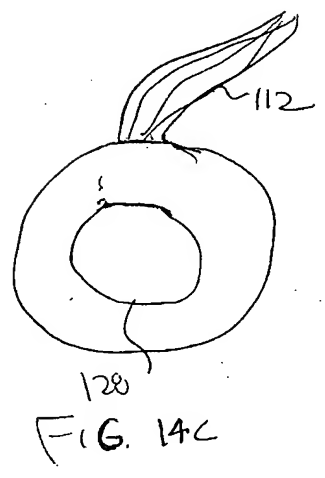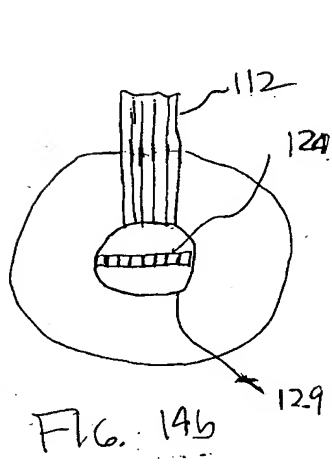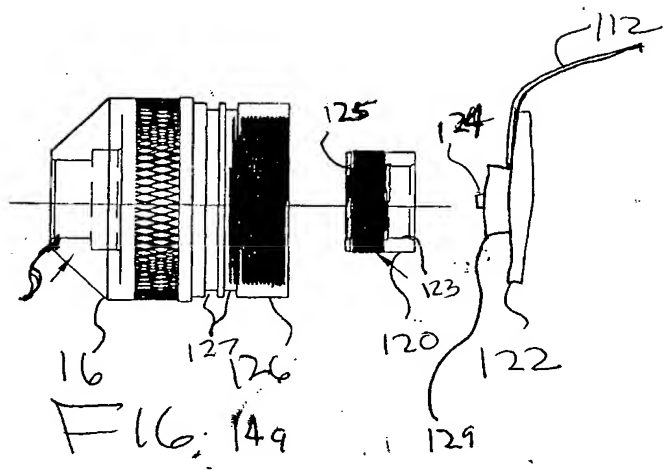


10072020-020602

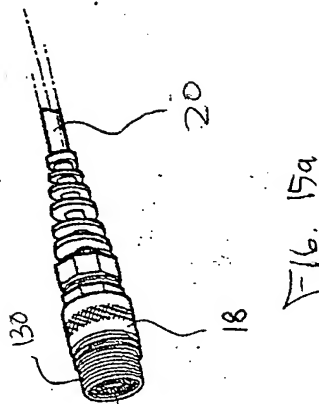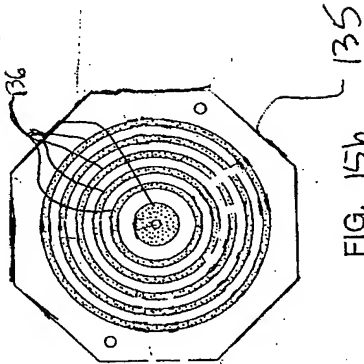

10072020-02022001

10072020-020502

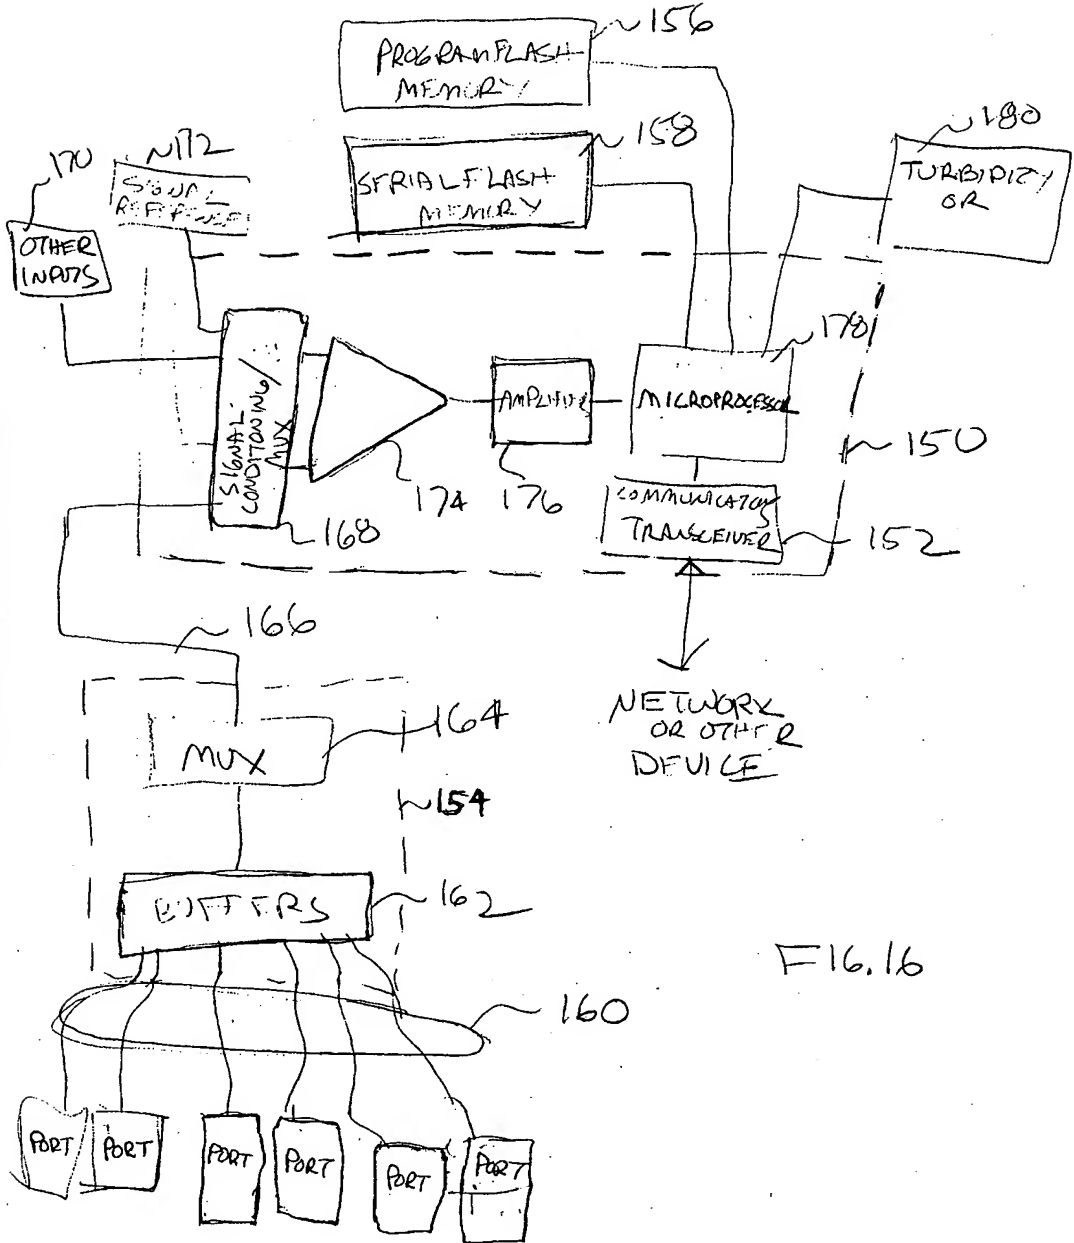

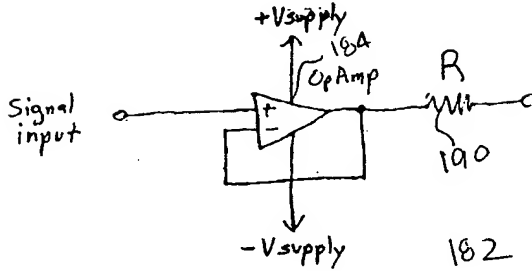


FIG. 17b

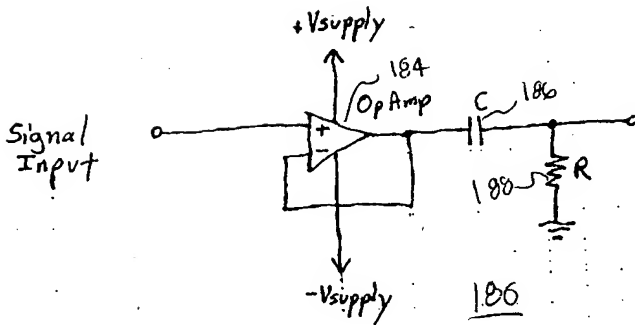


FIG. 17a

10072020-020602

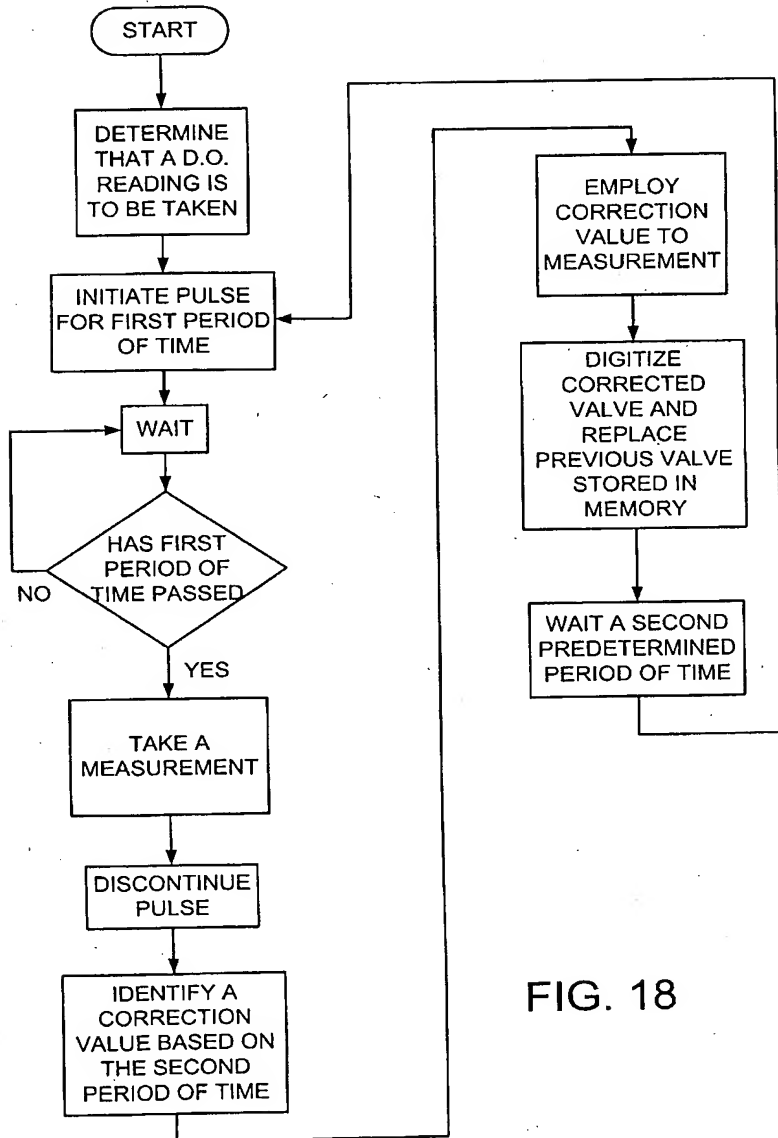


FIG. 18

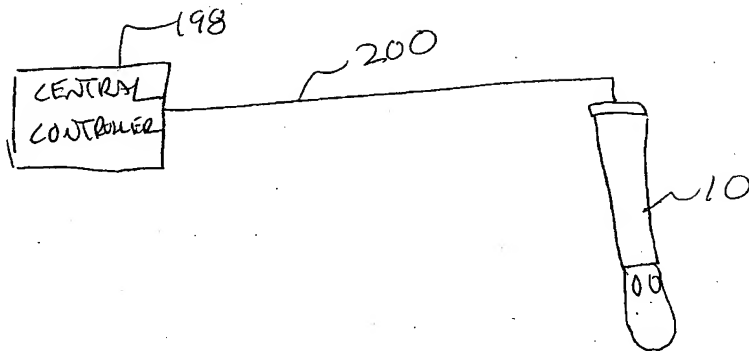


FIG. 19A

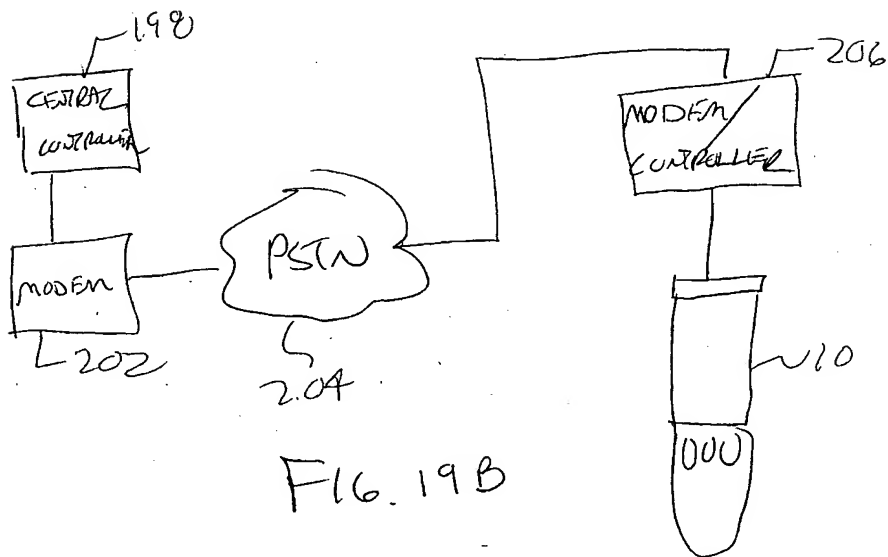


FIG. 19B

10072020-020602

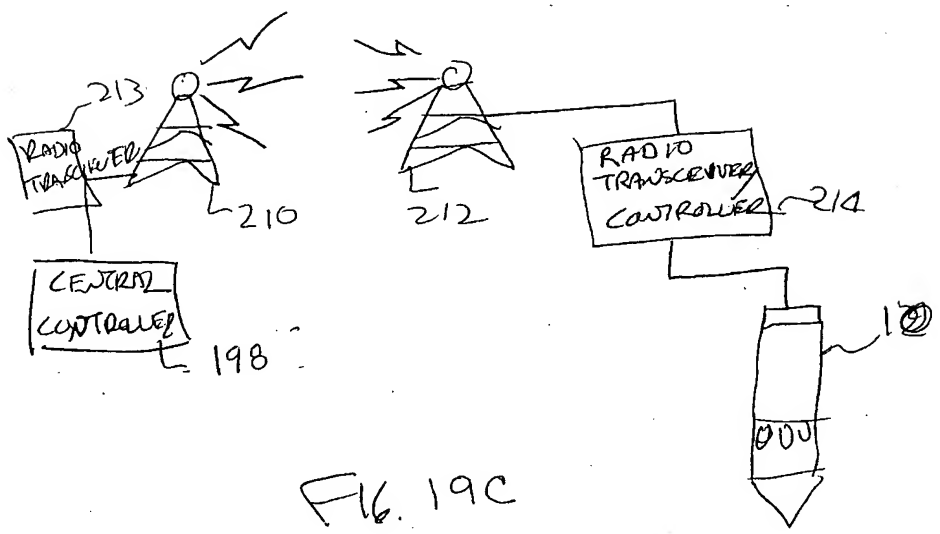


FIG. 19C

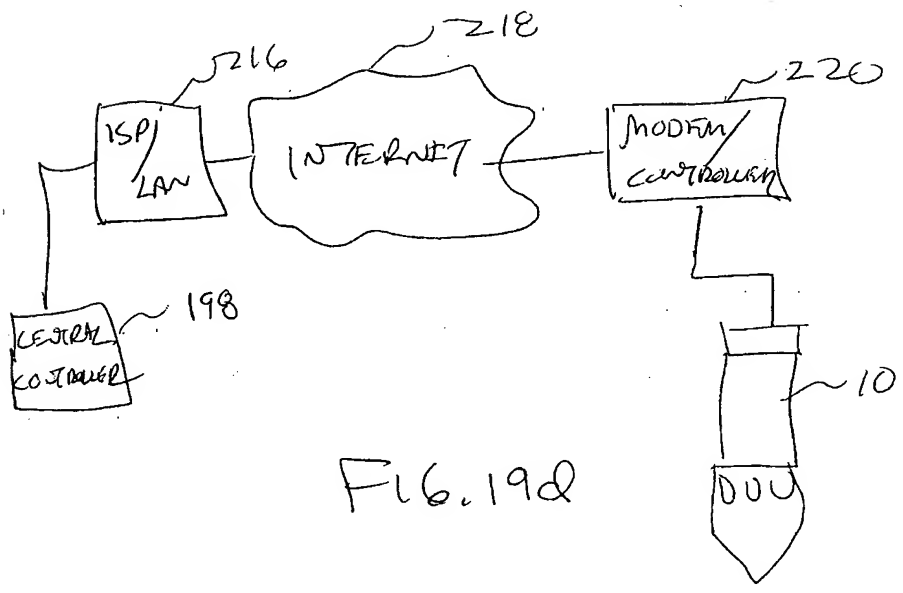


FIG. 19D

10072020-020502



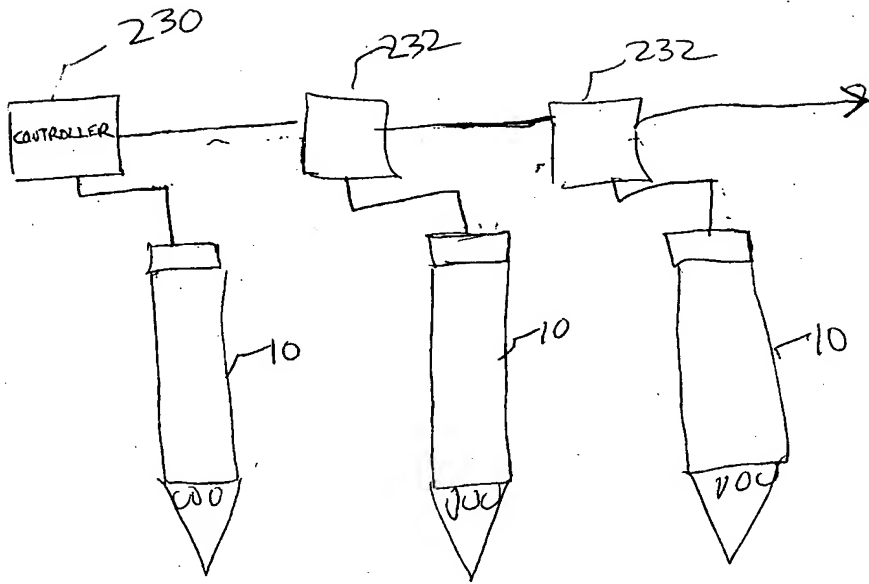


FIG. 20

10072020-020602

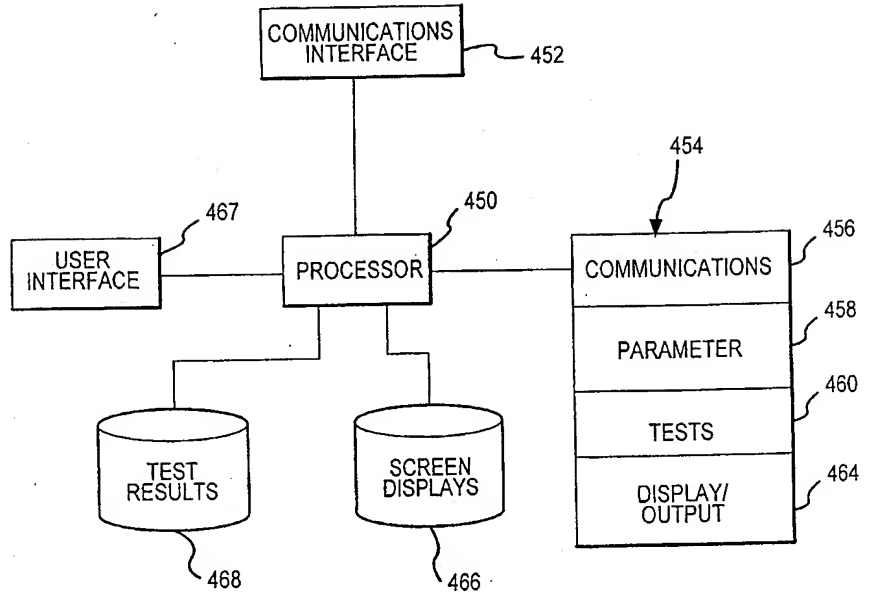


FIG. 21

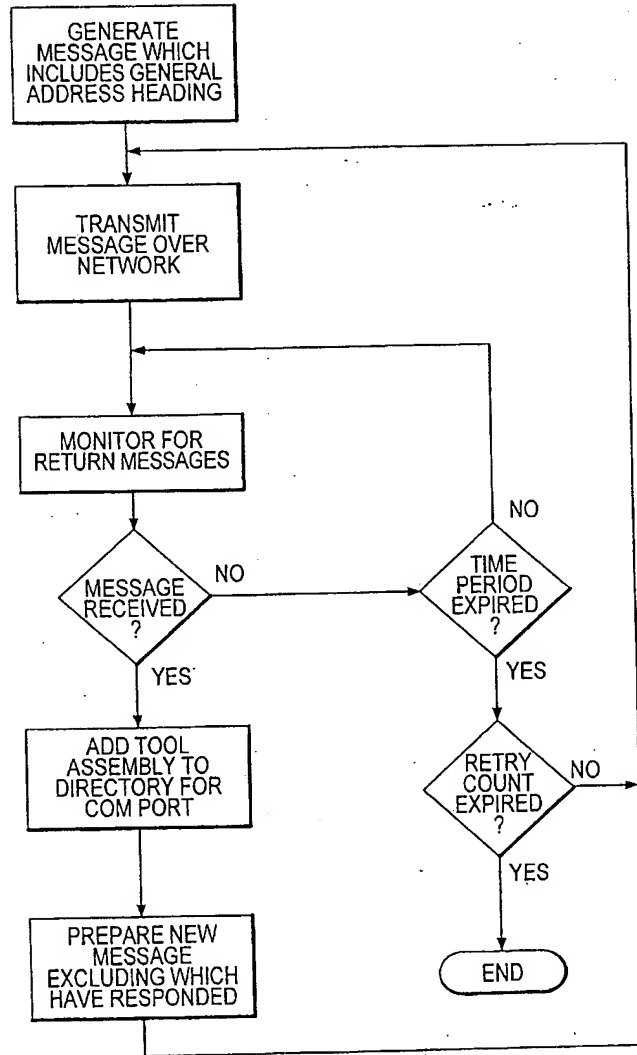


FIG. 22

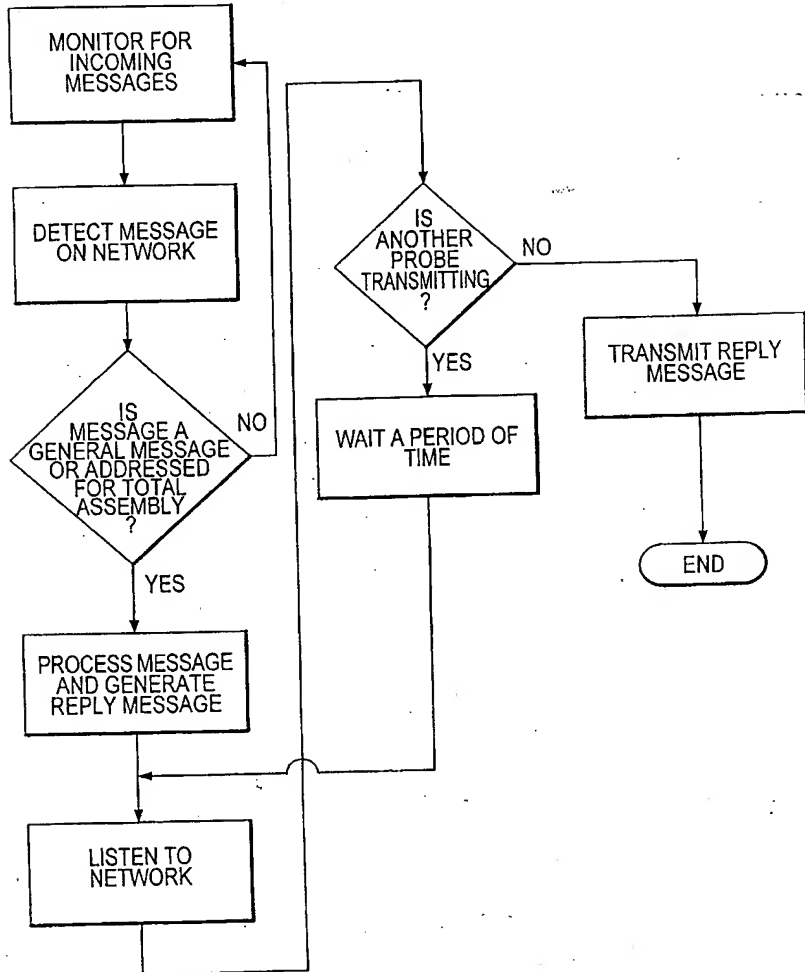


FIG. 23

10072020-020603

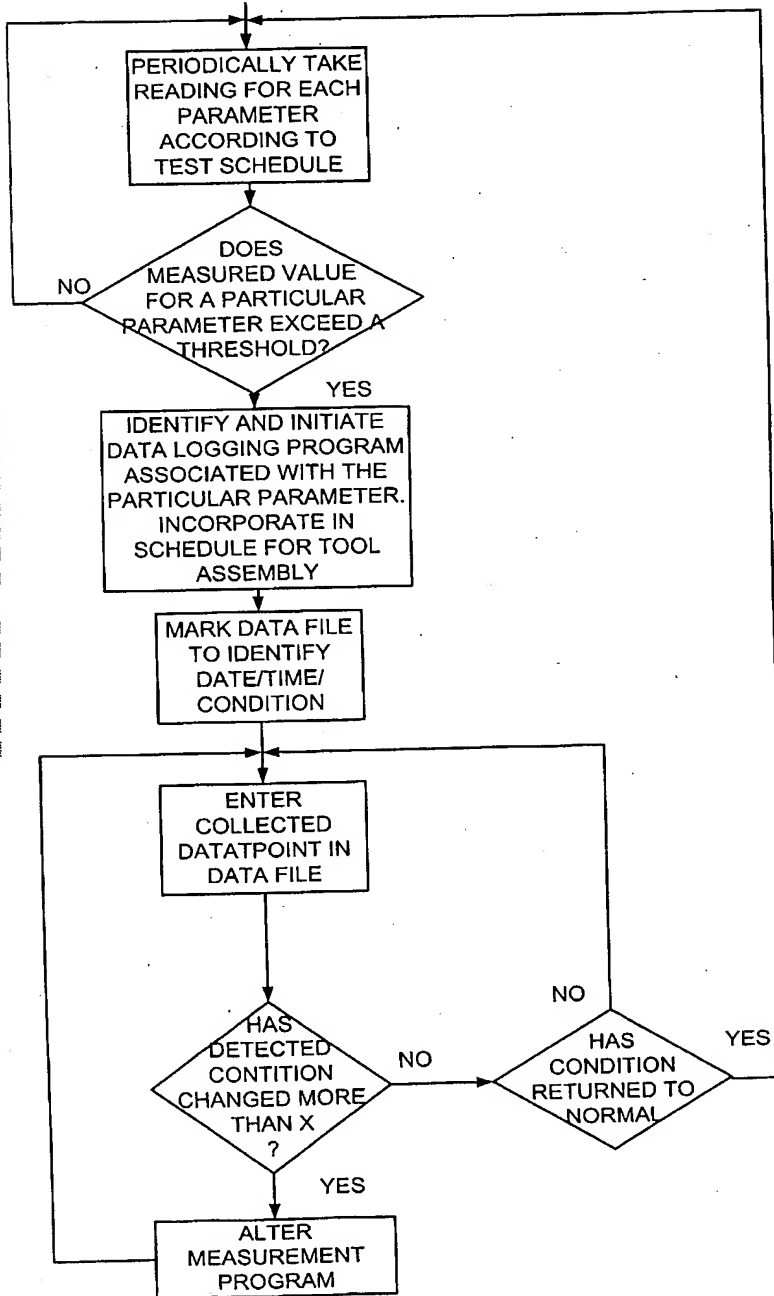


FIG. 24

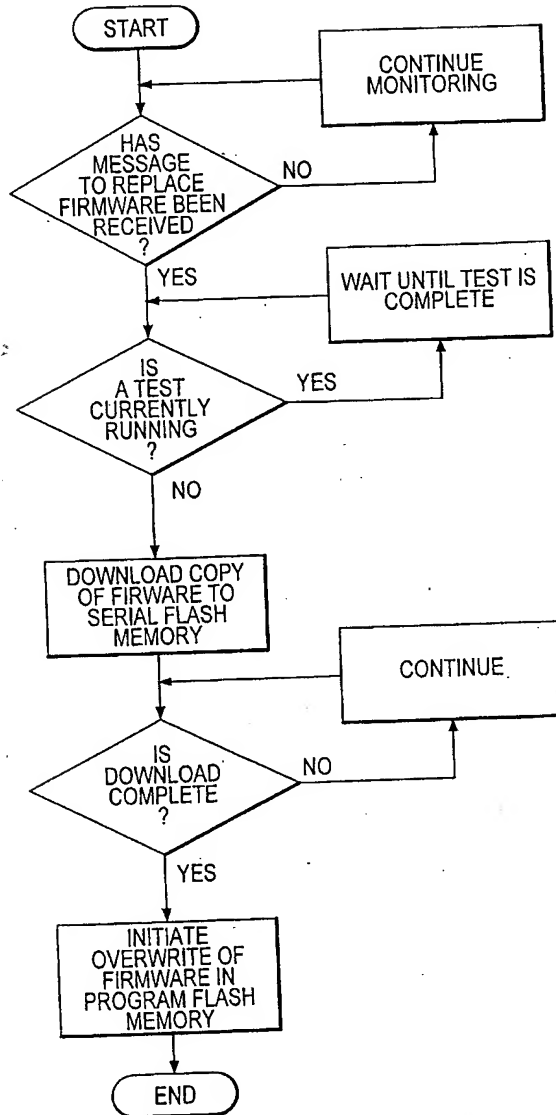


FIG. 25

10072020-020602